


<b>Monitor Accuracy</b>	
FiO <sub>2</sub>	± (2.5 vol. % + 2.5 % of the actual reading)
Flow	± (2 L/min + 10 % of the actual reading) (BTPS)
<b>Log</b>	
Type	Alarm, Operation
Max number	5000
<b>O<sub>2</sub> Sensor</b>	
Type	Galvanic fuel cell
Response time	< 15 s
<b>Communication interface</b>	
Communication interface	Rs232, Ethernet, VGA, USB port, Nurse call
<b>Gas supply</b>	
Gas type	O <sub>2</sub>
Pipe Connector	NIST or DISS
Gas supply pressure	280 - 600 kPa
Peak flow in case of single supply gas(air)	≥ 210 L/min (BTPS)*1
<b>Operation Data</b>	
<b>Environmental specifications</b>	
Temperature	5 - 40 °C (operating); -20 to 60 °C (storage and transport, O <sub>2</sub> sensor: -20 to 50°C)
Relative Humidity	10 - 95 % (operating); 10 - 95 % (storage and transport)
Barometric Pressure	62 - 106 kPa (operating); 50 -106 kPa (storage and transport)
<b>Power and Battery Backup</b>	
<b>External AC power supply</b>	
Input voltage	100 - 240 V
Input frequency	50/60 Hz
Input current	2.7 - 1.1 A
Fuse	T3.15 AH/250 V
<b>External DC power supply</b>	
Input voltage	12 V
Input current	15 A
<b>Internal battery</b>	
Number of batteries	One or Two
Battery type	Build-in Lithium-ion battery, 14.8 VDC, 5800 mAh
Battery run time	180 min (Powered by one new fully - charged battery in standard working condition)*2 360 min (Powered by two new fully - charged battery in standard working condition)
<b>Trolley</b>	
Dimensions	1039 mm*528 mm*544 mm
Weight	Approximately 20 kg
<b>Special Functions and procedures</b>	
Sigh	
100% O <sub>2</sub>	
Suction	
Manual breath	
Expiratory hold	
Inspiratory hold	
P0.1	
NIF	
PV - Tool	
PEEPi	
O <sub>2</sub> Therapy	

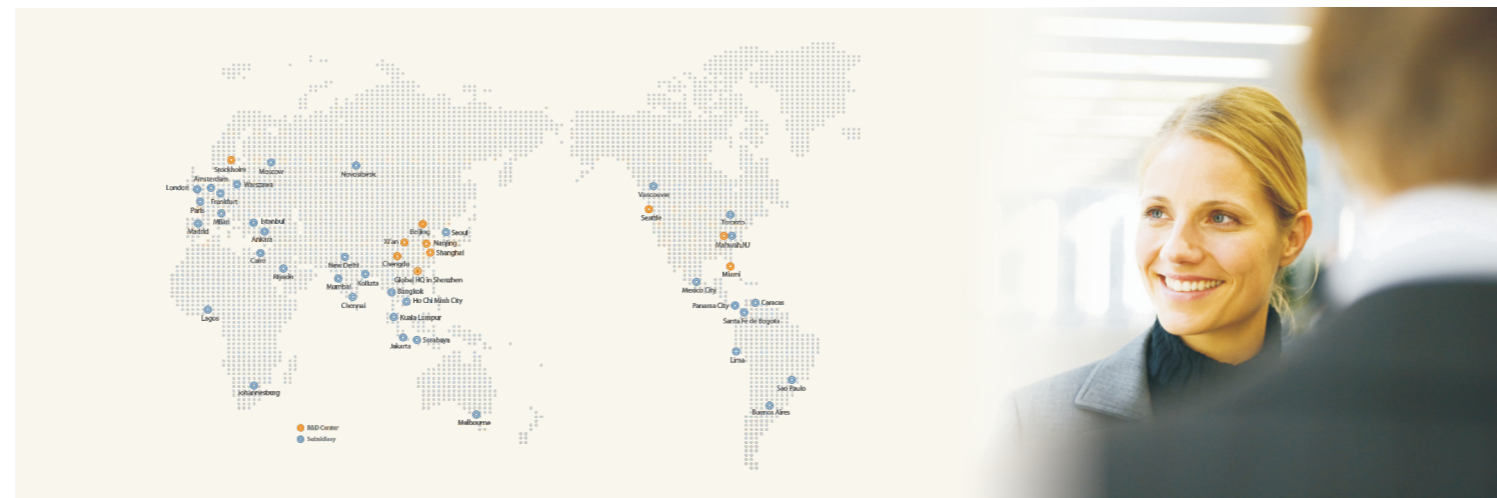


## Globally experienced, locally accessible

Mindray is one of the leading global providers of medical devices and solutions. Firmly committed to our mission of “sharing medical technologies with the world”, we are dedicated to innovation in the fields of Patient Monitoring & Life Support, In-Vitro Diagnostics, and Medical Imaging. The 1 Solution capitalizes on Mindray's broad product portfolio and offers hospitals a holistic and systemic solution to improve the overall efficiency and quality of care particularly in three key clinical areas: emergency care, peri-operative care, and critical care.

Headquartered in Shenzhen, China, and listed on the New York Stock Exchange, Mindray possesses a sound distribution and service network with subsidiaries in 18 countries in North and Latin America, Europe, Africa and Asia-Pacific. While improving the quality of care, we help in reducing its cost, making it more accessible to a larger part of humanity.

Since its foundation in 1991, Mindray's development has been driven by innovation. Mindray has built up a global R&D network with research centers in Seattle, New Jersey, Miami, Stockholm, Shenzhen, Beijing, Nanjing, Chengdu, Xi'an and Shanghai.

Today, Mindray's products and services can be found in healthcare facilities in over 190 countries and regions. Inspired by the needs of our customers, we adopt advanced technologies and transform them into accessible innovation, bringing healthcare within reach.

<p>Mindray Building, Keji 12th Road South, High-tech Industrial Park, Nanshan, Shenzhen 518057, P.R. China Tel: +86 755 8188 8998 Fax: +86 755 26582680 E-mail: intl-market@mindray.com www.mindray.com</p>	<p><b>mindray</b>   ———— are registered trademarks or trademarks owned by Shenzhen Mindray Bio-medical Electronics Co., LTD. © 2014 Shenzhen Mindray Bio-Medical Electronics Co., Ltd. All rights reserved. Specifications subject to changes without prior notice. P/N:ENG--SV 300 datasheet-210285x6P-20160301</p>
	

## SV300 Ventilator



<b>Technical Specifications</b>		
<b>Physical Specification</b>		
Dimensions	354 mm*315 mm*249 mm (Excluding the trolley)	
Weight	Approximately 10 kg (Excluding the trolley)	
<b>Screen</b>		
Display Size	12.1 Color active matrix TFT touch	
Display Resolution (H) x (V)	1280*800 pixels	
Brightness	Adjustable	
<b>Ventilation Specifications</b>		
Patient Type	Adults, children, infants (body weight of at least 3 kg)	
Ventilation Mode	V-A/C (Volume assist/control) P-A/C (Pressure assist/control) V-SIMV (Volume - Synchronized Intermittent Mandatory Ventilation) P-SIMV (Pressure - Synchronized Intermittent Mandatory Ventilation) DuoLevel (Duo Level Ventilation) CPAP (Continuous Positive Airway Pressure) PSV (Pressure Support Ventilation) APRV (Airway Pressure Release Ventilation) PRVC (Pressure Regulated Volume Control) PRVC-SIMV ((Pressure Regulated Volume Control- Synchronized Intermittent Mandatory Ventilation) NIV (Non-invasive ventilation) Apnea Ventilation	
<b>Controlled Parameters</b>		
O <sub>2</sub> %	21 - 100% (increments of 1 %)	
TV(Tidal Volume)	Adult: 100 - 3000 mL (increments of 10 mL) Pediatric: 20 - 300 mL (increments of 1 mL)	
f (Ventilation frequency)	1 - 150 bpm (increments of 1 bpm)	
fSIMV (Ventilation frequency in SIMV mode)	1 - 60 bpm (increments of 1 bpm)	
I:E range	4:1 - 1:10 (99:1-1:99 in DuoLevel mode, increments of 0.5)	
Tinsp (Inspiratory time)	0.20 - 10 s (increments of 0.05 s)	
Tslope (Time of Pressure Rising)	0 - 2.00 s (increments of 0.05 s)	
Thigh	0.2 - 30 s (increments of 0.1 s)	
Tlow	0.2 - 30 s (increments of 0.1 s)	
Tpause	5 % - 60 % (increments of 5 %), Off	
ΔPinsp	5 - 80 cmH <sub>2</sub> O (increments of 1 cmH <sub>2</sub> O)	
ΔPsupp	0 - 80 cmH <sub>2</sub> O (increments of 1 cmH <sub>2</sub> O)	
Phigh	0 - 80 cmH <sub>2</sub> O (increments of 1 cmH <sub>2</sub> O)	
Plow	0 - 45 cmH <sub>2</sub> O (increments of 1 cmH <sub>2</sub> O)	
PEEP	0 - 50 cmH <sub>2</sub> O (increments of 1 cmH <sub>2</sub> O)	
Flow trigger	0.5 -15 L/min (increments of 0.1 L/min), Off	
Pressure trigger	-10 to - 0.5 cmH <sub>2</sub> O (increments of 0.5 cmH <sub>2</sub> O), Off	
Exp% (Expiration termination level)	10 - 85% (increments of 5%), Auto	
Inspiratory waveform	Square, Decelerating	
<b>Apnea Ventilation</b>		
Tvapnea	Adult: 100 - 2000 mL (increments of 10 mL)	Pediatric: 20 - 300 mL (increments of 1 mL)
ΔPapnea	5 - 80 cmH <sub>2</sub> O (increments of 1 cmH <sub>2</sub> O)	
fapnea	1 - 80 bpm (increments of 1 bpm)	
Apnea Tinsp	0.20 - 10 s (increments of 0.05 s)	

\*1 BTPS =Body Temperature and Pressure Saturated

\*2 The standard work condition is: Ventilation mode: P-A/C; ΔPinsp: 10 cmH<sub>2</sub>O; f: 10 bpm; Tinsp: 2 s; Tslope: 0.2 s; O<sub>2</sub>: 21 Vol.%; PEEP: 5 cmH<sub>2</sub>O; R: 20 cmH<sub>2</sub>O/L/s; C: 20 ml/cmH<sub>2</sub>O; Gas supply nominal work pressure: 400±100 kPa.

<b>Sigh</b>	
Sigh Switch	ON, Off
Interval	20 s - 180 min (increments of 1 s from 20 to 59 s, increments of 1 min from 1 to 180 min)
Cycles Sigh	1 - 20 (increments of 1 )
Δint.PEEP	1 - 45 cmH <sub>2</sub> O (increments of 1 cmH <sub>2</sub> O), Off
<b>Automatic Tube Resistance Compliance</b>	
Tube Type	ET Tube, Trach Tube, Disable ATRC
Tube I.D.	Adult: 5.0 - 12.0 mm (increments of 0.5 mm) Pediatric: 2.5 - 8.0 mm (increments of 0.5 mm)
Compensate	0 -100 % (increments of 1 %)
Expiration Compliance Switch	ON, Off
<b>Monitored parameters</b>	
Airway pressure range	Ppeak, Pplat, Pmean, PEEP (Range 0 - 120 cmH <sub>2</sub> O)
Tidal volume range	TVi, TVe, TVe/IBW (Range 0 - 4000 mL)
Frequency range	ftotal, fmand, fspn (Range 0 - 200 bpm)
Minute volume range	MV, MVspn, MVleak (Range 0 - 100 L/min)
Resistance	Rinsp, Rexp (0 - 600 cmH <sub>2</sub> O/L/s)
Compliance	Cstat, Cdyn (0 - 300 mL/cmH <sub>2</sub> O)
Inspired Oxygen(FiO <sub>2</sub> )	15 - 100 %
RSBI	0 - 999 1/(L-min)
WOB	0 - 100 J/min
P0.1	-20 - 0 cmH <sub>2</sub> O
NIF	-45 - 0 cmH <sub>2</sub> O
PEEPi	0 - 80 cmH <sub>2</sub> O
Rcexp	0 - 10 s
TVe/IBW	0 - 50 ml/kg
MV/IBW	0 -33.3 L/(min-kg)
I:E	100:1 -1:150
Tinsp	0.00 - 99 s
Texp	0.00~99 s
Insp Flow	0~300 L/min
Exp Flow	0~180 L/min
Tube Leak%	0~100%
Waveforms	Airway pressure - time, Flow - time, Volume - time
Loops	Paw - Volume, Flow - Volume, Paw - Flow
<b>Ventilator Accuracy</b>	
<b>Control Accuracy</b>	
O <sub>2</sub> %	± (3 vol.% +1 % of setting)
TV	± (10 mL + 10 % of setting) (BTPS)
Tinsp	± 0.1 s or ± 10 % of setting, whichever is greater
I: E	2: 1 to 1: 4: ± 10 % of setting, other range: ± 15% of setting
f	± 1 bpm
fSIMV	± 1 bpm
Tslope	± (0.2 s + 20 % of setting)
PEEP/ΔPinsp/ΔPsupp /Phigh/Plow	± (2.0 cmH <sub>2</sub> O + 5 % of setting)
Thigh	± 0.2 s or ± 10 % of setting, whichever is greater
Tlow	± 0.2 s or ± 10 % of setting, whichever is greater
Pressure Trigger	± (1.0 cmH <sub>2</sub> O + 10 % of setting)
Flow Trigger	± (1.0 L/min + 10 % of setting)
Δint.PEEP	± (2.0 cmH <sub>2</sub> O + 5% of setting)
fapnea	± 1 bpm
ΔPapnea	± (2.0 cmH <sub>2</sub> O + 5 % of setting)
TVapnea	± (10 mL + 10 % of setting) (BTPS)
Apnea Tinsp	± 0.1 s or ± 10% of setting, whichever is greater

<b>Monitoring Accuracy</b>	
Airway pressure (Ppeak, Pplat, Pmean, PEEP )	± (2 cmH <sub>2</sub> O + 4 % of the actual reading)
Tidal Volume (TVi, TVe, TVe/IBW, TVe spn)	0 ml - 100 ml: ± (10 ml + 3 % of the actual reading) (BTPS); 100 ml - 4000 ml: ± (3 ml + 10 % of the actual reading) (BTPS)
Minute Volume (MV, MVspn, MVleak)	± (0.2 L/min + 10 % of the actual reading) (BTPS)
Frequency (ftotal, fmand, fspn)	± 5% of reading or ± 1bpm, whichever is greater
Inspired Oxygen (FiO <sub>2</sub> )	± (2.5 vol.% + 2.5 % of the actual reading)
Resistance	0 to 20: ± 10 cmH <sub>2</sub> O/L/s Other range: 50 % of actual reading
Compliance	± (2 ml/cmH <sub>2</sub> O + 20 % of the actual reading)
RSBI	± (3 1/(L-min))+15% of the actual reading)
WOB	± (1 J/min+15% of the actual reading)
NIF	± (2 cmH <sub>2</sub> O + 4 % of the actual reading)
P0.1	± (2 cmH <sub>2</sub> O + 4 % of the actual reading)
PEEPi	No declaration
RCexp	± (0.2 s + 20 % of the actual reading)
<b>Alarm settings</b>	
Tidal Volume	High Adult: 110 - 4000 mL, Off Pediatric: 25 - 600 mL, Off Low Adult: 50 - 4000 ml, Off Pediatric: 5 - 600 mL, Off
Minute Volume	High Adult: 0.2 - 100.0 L/min Pediatric: 0.2 - 60.0 L/min Low Adult: 0.1 - 50.0 L/min Pediatric: 0.1 - 30.0 L/min
Air pressure	High 10 - 85 cmH <sub>2</sub> O Low PEEP+4 cmH <sub>2</sub> O
Frequency	High 1 - 200 bpm, Off Low 1 - 200 bpm, Off
Inspired oxygen (FiO <sub>2</sub> )	High Auto, internal alarm limit: min (set value+max (7 % or set value*10 %), 100 %) Low Auto,internal alarm limit: max (set value-max (7 % or set value*10 %),18 %), Absolute FiO <sub>2</sub> low limit: 18 %
Apnea alarm time	5 - 60 s
<b>SideStream CO<sub>2</sub> Module (optional)</b>	
Displayed numerics	EtCO <sub>2</sub>
Measurement Range	0 - 99 mmHg
Measurement accuracy	0 to 40 mmHg ± 2 mmHg 41 to 76 mmHg ± 5% of reading 77 to 99 mmHg ± 10% of reading
Waveforms	EtCO <sub>2</sub> - time
Resolution	1 mmHg
Sampling rate	Adult: 70 ml/min, 100 ml/min, 120 ml/min, 150 ml/min Pediatric: 70 ml/min, 100 ml/min
Sampling rate Accuracy	± 15% of the set value or ± 15 mL/min, whichever is greater
System response time	Using Adult water trap, Adult sampling line: < 7.5 s @ 150 ml/min < 8.0 s @ 120 ml/min < 8.5 s @ 100 ml/min < 9.5 s @ 70 ml/min Using Pediatric water trap, Pediatric sampling line: < 7.5 s @ 100 ml/min < 8.0 s @ 70 ml/min
Rise time	Adult water trap: < 400 ms @70 ml/min < 330 ms @100 ml/min < 300 ms @120 ml/min < 240 ms @150 ml/min Pediatric water trap: < 400 ms @70 ml/min < 330 ms @100 ml/min
Water trap cleaning time	Adult water trap: ≥24 h @150 ml/min ≥48 h @70 ml/min Pediatric water trap: ≥24 h @100 ml/min ≥48 h @70 ml/min

<b>Sidestream CO<sub>2</sub> alarm limits</b>	
EtCO <sub>2</sub>	High 2 - 99 mmHg Low 0 - 97 mmHg
<b>MainStream CO<sub>2</sub> Module(optional)</b>	
Displayed numerics	EtCO <sub>2</sub>
EtCO <sub>2</sub> Measurement range	0 -150 mmHg
EtCO <sub>2</sub> Measurement Accuracy	0 to 40 mmHg ± 2 mmHg of reading 41 to 70 mmHg ± 5% of reading 71 to 100 mmHg ± 8% of reading 101 to 150 mmHg ± 10% of reading
Resolution	1 mmHg
Waveforms	EtCO <sub>2</sub> - time, Volume - EtCO <sub>2</sub>
<b>Other Parameters</b>	
SlopeCO <sub>2</sub> (slope of the alveolar plateau)	Range: 0 - 9.99 %/L Resolution: 0.01 %/L
Vtalv (Alveolar tidal ventilation)	Range: 0 - 9999 ml Resolution: 1 ml
V'alv (Alveolar minute ventilation)	Range: 0 - 20 L/min Resolution: 0.01 L/min for < 1 L/min, 0.1 L/min for ≥ 1 L/min
V'CO <sub>2</sub> (CO <sub>2</sub> elimination)	Range: 0 - 9999 mL/min Resolution: 1 ml/min
VDaw (Airway death space)	Range: 0 - 999 mL Resolution: 1 ml
VDaw/TVe (Physiological dead space fraction at the airway opening)	Range: 0 - 100 % Resolution: 1 %
VeCO <sub>2</sub> (exhaled CO <sub>2</sub> volume)	Range: 0 - 999 mL Resolution: 1 ml
ViCO <sub>2</sub> (inspired CO <sub>2</sub> volume)	Range: 0 - 999 mL Resolution: 1 ml
System response time	< 2.0 s
<b>CO<sub>2</sub> alarm limits</b>	
EtCO <sub>2</sub>	High 2 - 150 mmHg Low 0 - 148 mmHg
<b>SpO<sub>2</sub> module(optional)</b>	
<b>Measurement Range and Resolution</b>	
SpO <sub>2</sub>	Range: 0 - 100 % Resolution: 1 %
PR	Range: 20 - 254 1/min Resolution: 1 1/min
PI	Range: 0.05 - 20 %
<b>Measurement Accuracy</b>	
SpO <sub>2</sub>	70 to 100 %: ±2 % 0 % to 69 %: Not specified.
PR	± 3 1/min
<b>SpO<sub>2</sub> alarm limits</b>	
SpO <sub>2</sub>	High 2 -100 % Low 0 - 98 %
	Desat 0 - 98 %
PR	High 17 - 300 1/min Low 15 - 298 1/min
<b>Trend</b>	
Type	Tabular, Graphic
Length	72 hours
Content	Monitor Parameters, Setting Parameters (Setting Ventilation mode and Parameters)
<b>O<sub>2</sub> Therapy</b>	
<b>Controlled Parameters</b>	
O <sub>2</sub> %	21 - 100 % (increments of 1 %)
Flow	2 - 50 L/min
<b>Controlled Accuracy</b>	
O <sub>2</sub> %	± (3 vol.% +1 % of setting)
Flow	± (2 L/min +10 % of setting) (BTPS)